

TITLE: METHOD FOR CONTROLLING POSITION OF MEDICAL INSTRUMENTS INVENTOR: GARY L. LONG, et al.

DOCKET: END-838

ATTY: GERARD S. GRESSEL; PHONE: (513) 337-3535

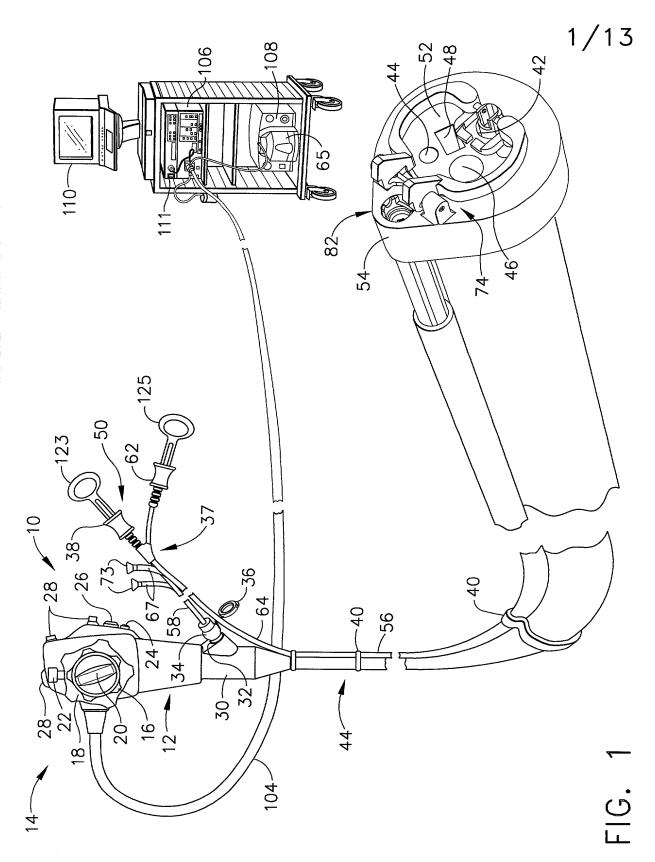


TITLE: METHOD FOR CONTROLLING POSITION OF MEDICAL INSTRUMENTS INVENTOR: GARY L. LONG, et al.
DOCKET: END-838
ATTY: GERARD S. GRESSEL; PHONE: (513) 337-3535

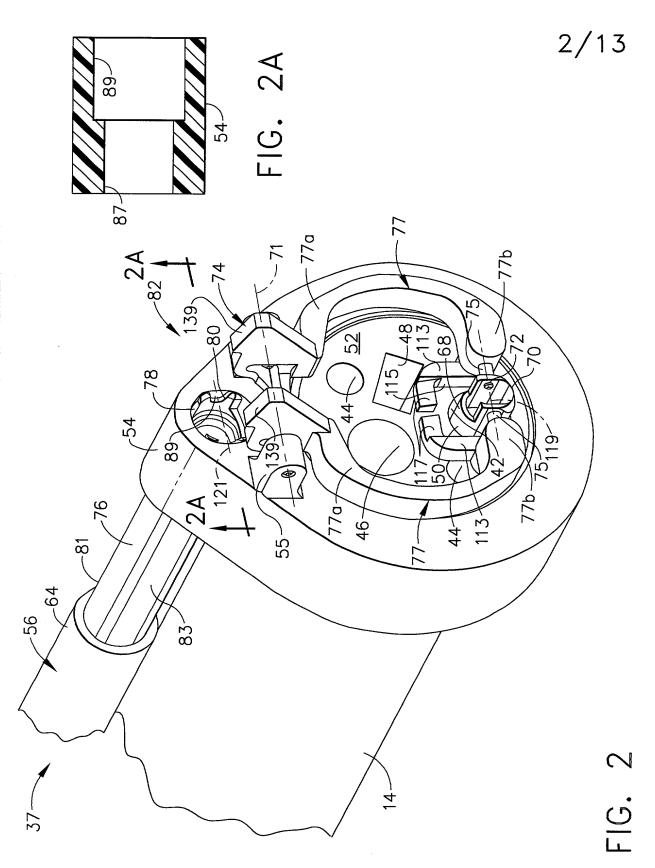


DOCKET: END-838
ATTY: GERARD S. GRESSEL; PHONE: (513) 337-3535




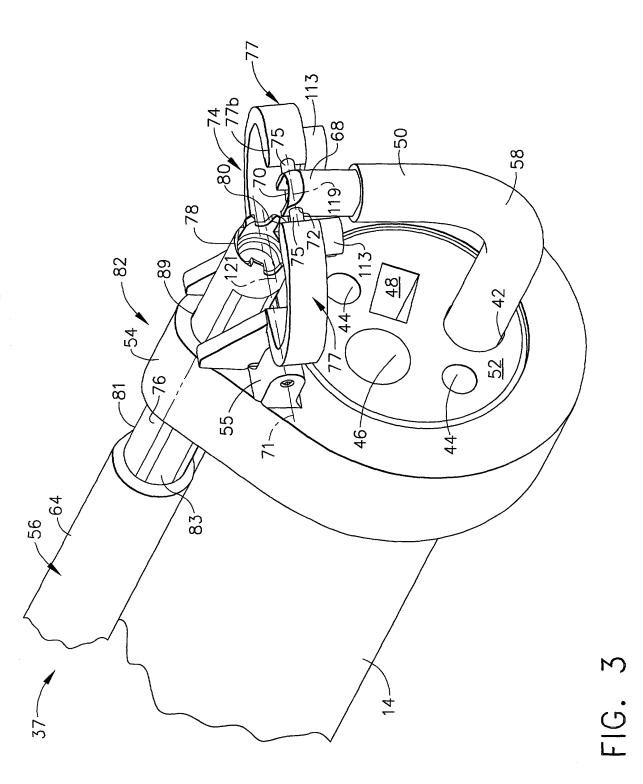




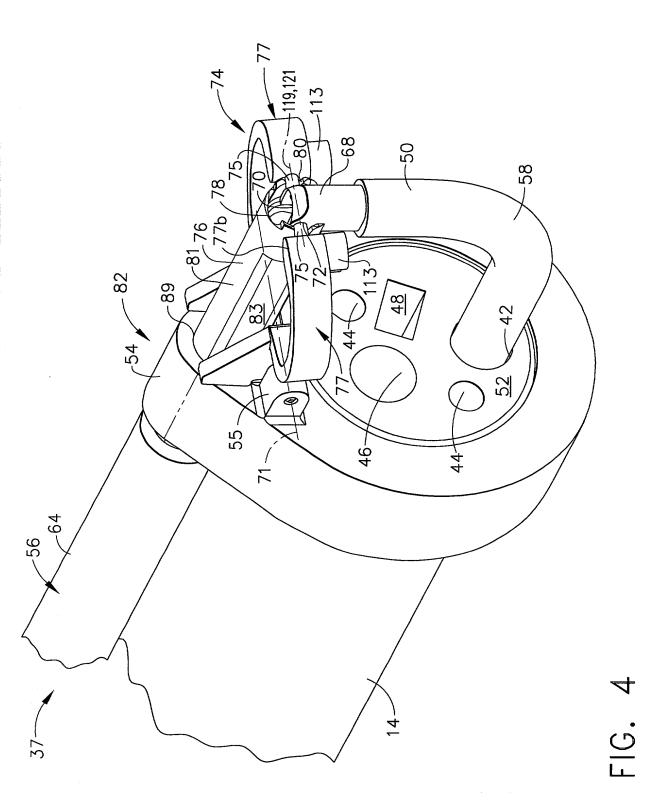

DOCKET: END-838
ATTY: GERARD S. GRESSEL; PHONE: (513) 337-3535

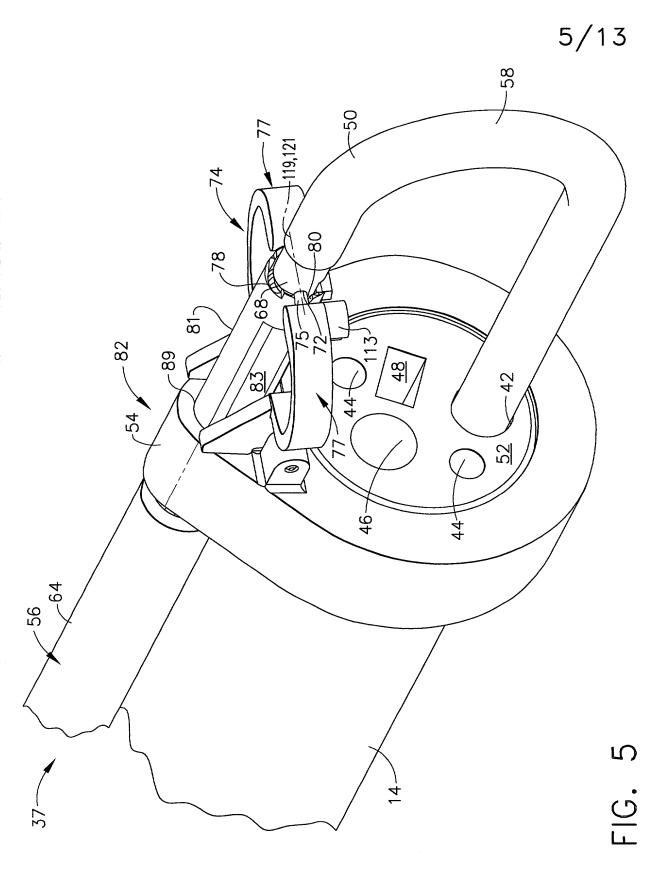

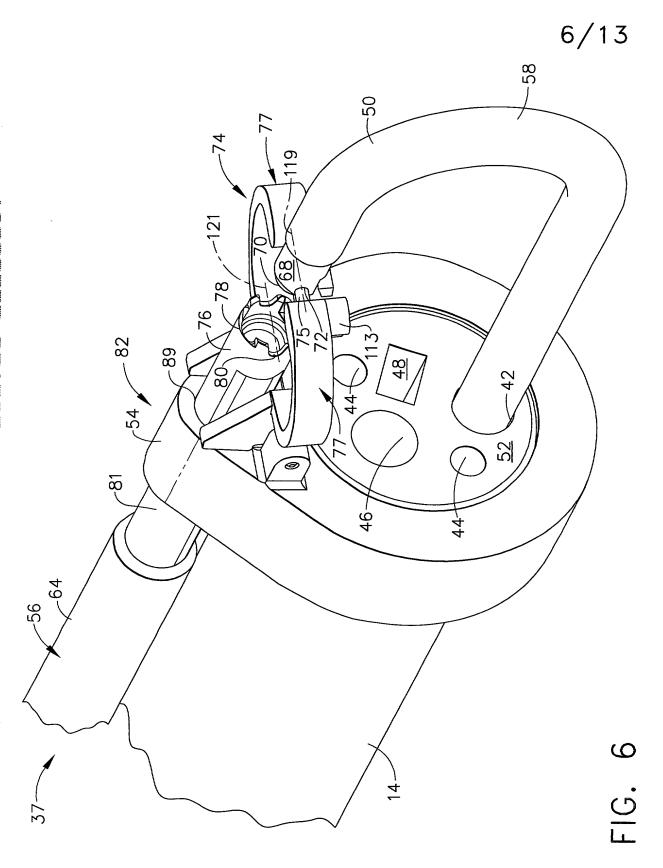

DOCKET: END-838

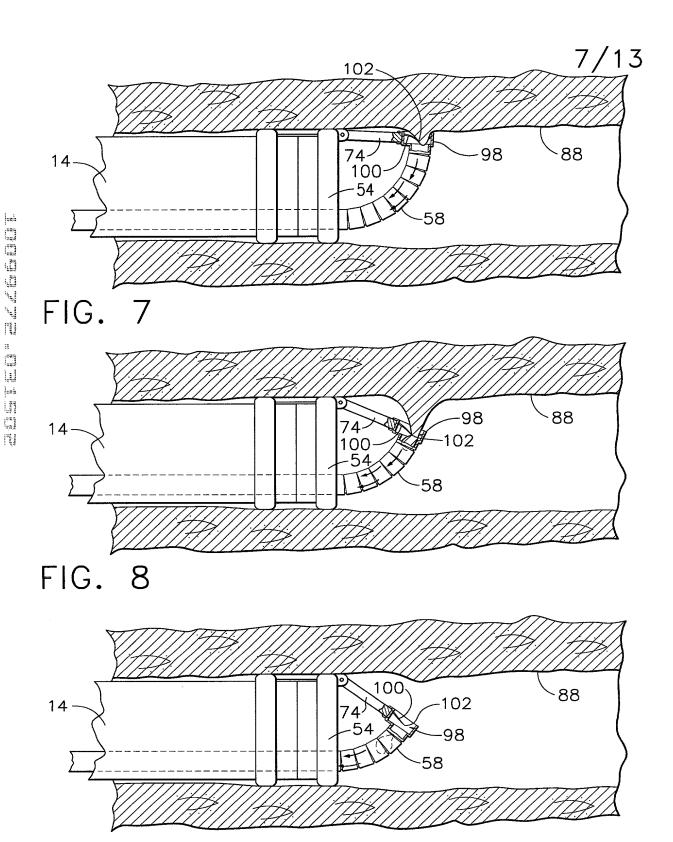


FIG. 9

DOCKET: END-838

ATTY: GERARD S. GRESSEL; PHONE: (513) 337-3535

8/13

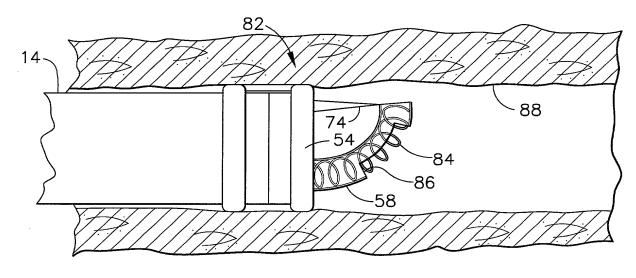


FIG. 10

The state of the s

The state of the s

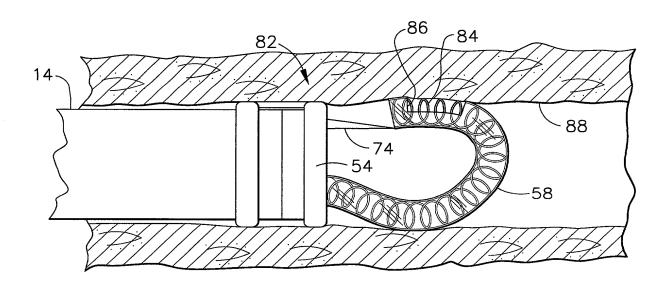


FIG. 11

DOCKET: END-838
ATTY: GERARD S. GRESSEL; PHONE: (513) 337-3535

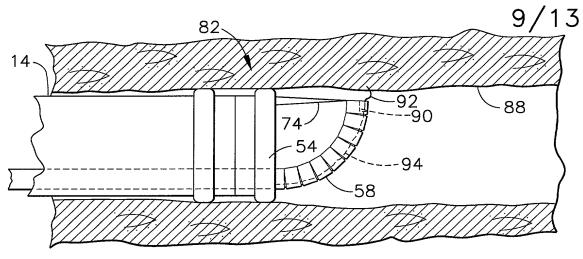


FIG. 12

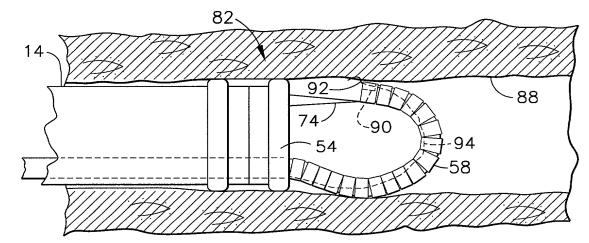


FIG. 13

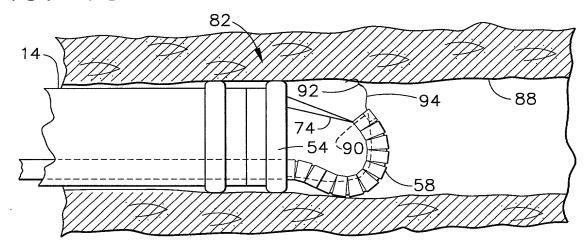


FIG. 14

DOCKET: END-838

ATTY: GERARD S. GRESSEL; PHONE: (513) 337-3535

10/13

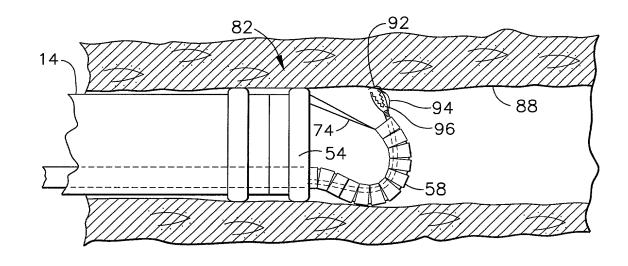


FIG. 15

The state of the s

Henry Livery many

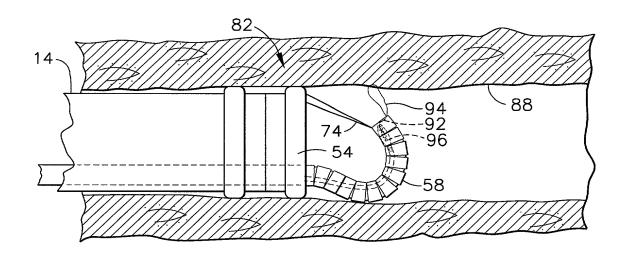
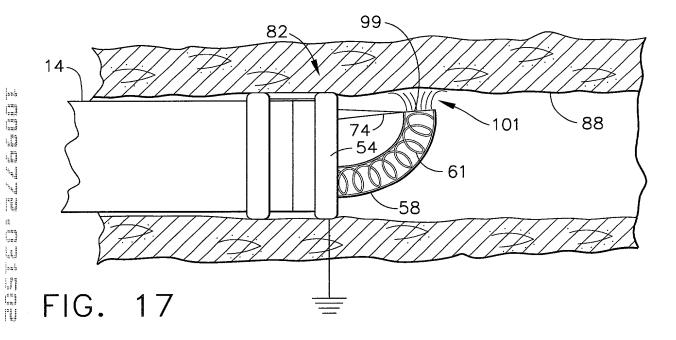


FIG. 16

ATTY: GERARD S. GRESSEL; PHONE: (513) 337-3535

11/13



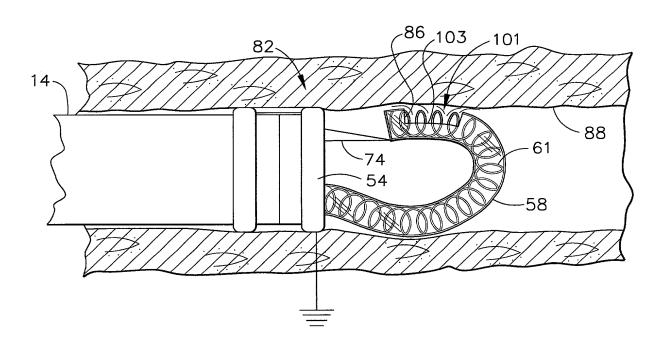


FIG. 18

DOCKET: END-838

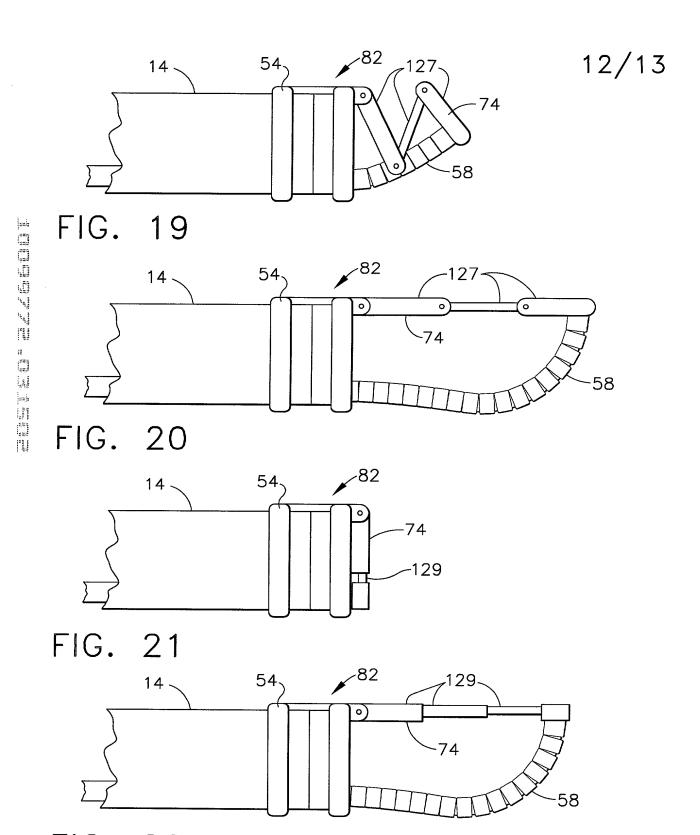


FIG. 22

DOCKET: END-838 ATTY: GERARD S. GRESSEL; PHONE: (513) 337-3535

13/13

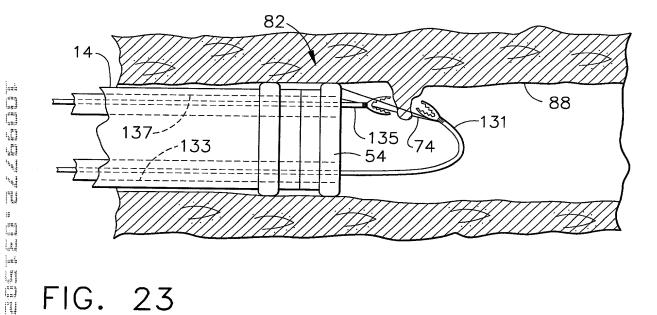


FIG. 23

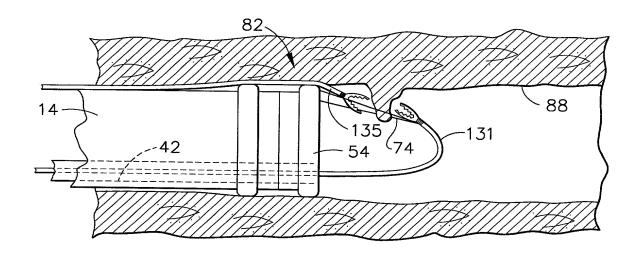


FIG. 24